

# Development of the Electronics for a Gait Retraining Device

Kimmy Migel, Rima Patel, Pradham Tanikella, Stefan Lehman, Kit Williams, and Nathan Smith

UNC-Chapel Hill, Chapel Hill, NC

## 1. Tested the Existing Prototype

The electronics team began by working with the initial prototype to evaluate how to improve the device. The initial prototype was developed to trigger a vibration motor when a pressure threshold is surpassed on the lateral side of the foot. After evaluating the prototype the electronics team established an objective of optimizing the electrical circuit towards testing usability as well as proper and reliable functionality.


### OBSERVATIONS

- Two potentiometers create a threshold, one as a reference and the other to assign a relative voltage threshold value needed to turn on the motor.
- The voltage depends on the force exerted on a force-sensitive resistor (FSR) attached to the bottom of the subject's foot
- Accomplished the desired behavior to set a threshold for a motor, dependent on the changing weight the subject exerts on the FSR.

### PROBLEMS

- Establishing a threshold for each subject became very subjective
- Potentiometers would each need to be constantly adjusted without any specific or knowable placement.
- A reoccurring issue with setting threshold values for each individual
- Electrical components became unattached when the subject would walk
- The bulky design additionally made data collection difficult when trying to track walking patterns

### INITIAL PROTOTYPE

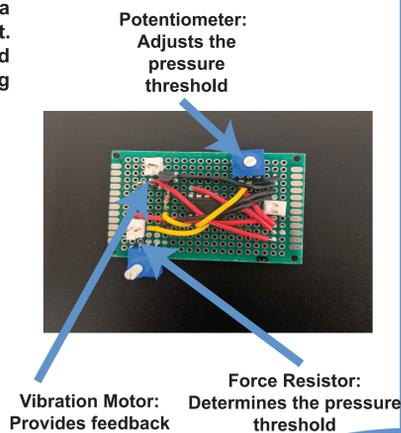

## 2. Redesigned Circuit

The goal of the redesign was to simplify the circuit to include fewer parts, make it easier to use, and secure the connections while maintaining its original function. Although the redesigned circuit was successful and more sensitive to various individual users, it still faced various issues.

### GOALS

- Make the device easily adjustable for each person.
- Replace the operational amplifier with an LM311 comparator to conduct the comparison between the FSR signal and a reference signal.
- Remove a potentiometer and replace it with a single resistor
- Limit the device to a single varying part.
- Soldered to a board to prevent wires from coming loose.

### PROBLEMS

- The device was not user-friendly
- Required manual changing of the physical potentiometer
- Still possessed a poor FSR connection, resulting in misreadings and frequent replacements of the FSR.


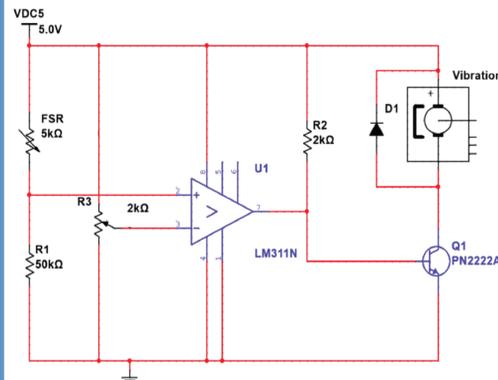


Figure 1. Redesigned Circuit Schematic.

## Gait Retraining for Lateral Ankle Sprains

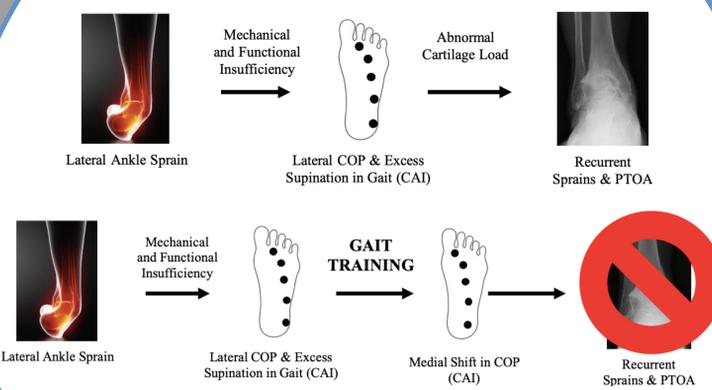

## 3. Added Microcontroller

The microcontroller has various capabilities to both take in and send out a signal based on the code that is integrated within it. Although we were able to achieve many more capabilities with the microcontroller, we still lacked ease of use for any person to use the device on their own without manipulating the device.

### GOALS

- Remove physical interactions needed with a potentiometer
- Be able to enter exact threshold
- Simplify circuit down to just a microcontroller and FSR
- Provide easy access for data extraction
- Bridge gap towards a mobile app

### PROBLEMS

- Code needed to be modified for each person
- Needed to add a motor drive circuit with a separate power source to drive the vibration motor



Figure 2. Teensy 3.2 USB Development Board used in the circuitry of the device

## 5. Developments

The final functional circuit utilizes microcontroller and Bluetooth capabilities and has been successfully tested to operate as intended. After trying different layouts, we eventually determined that a flat single layered layout was ideal. Further issues arose when trying to ensure a steady battery connection to the circuit. These issues have been resolved and functional prototypes have been constructed for clinical testing. However to be implemented in a real world testing setting, the circuitry needs to be compact and durable to be attached to the ankle.

### GOALS

- Portable, lightweight, rechargeable
- Can be fully implemented throughout a day
- "App" collection through android serial bluetooth (provided to user)
- Threshold set and adjusted based on person
- Translate the voltage output of the force sensor to an equivalent force measurement
- The design of the prototype connected to the side of the shoe rather than interfaced on top of the laces to provide the user with a more ergonomic interface

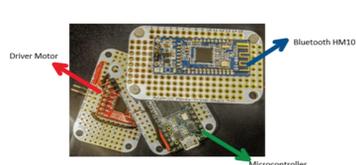


Figure 4. Three tier circuit




Figure 5. Final optimized circuit

### PROBLEMS

- Three tiers cause problems of wires breaking and difficult to troubleshoot issues
- Moving towards newer single board implementation
- Battery power incompatible with circuit elements = voltage regulator
- Durability of the connection of the battery pack to the electrical circuit. Wire connection fraying
- Voltage output in the single board circuit was not constant. The desired voltage throughout the board was 6 volts, but the actual measured value circuit was less than 3 volts

## 4. Added Bluetooth

To allow the app the ability to extract data and quantitatively present the progress of the subject, it was essential to add a Bluetooth connection. Establishing a connection is the first step moving towards long term functionality beyond the lab setting.

### GOALS

- Establish communication between the app and the device
- Add a DSD TECH HM-10 Bluetooth 4.0 to the circuit due to its easy implementation and compact size
- Alter code to have the threshold value be set and changed with the app instead of hardcoded into the Arduino
- Alter code to allow for the microcontroller to "listen" for incoming data

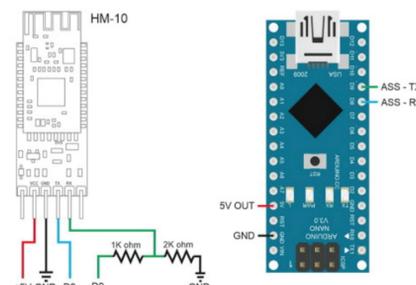


Figure 3. Schematic of the DSD TECH HM-10 Bluetooth 4.0 used to establish a bluetooth connection

## 6. Future Plans

We aim to provide a visual interface with realtime feedback through the development of a phone application. We plan to keep improving the prototype until there is seamless communication between the wearable component and the future phone application. In order to improve the physical prototype, the soldered circuit board will be made into a designed printed circuit board. New FSR's will be tested in order to select a sensor that is durable enough for constant wear. The next iteration of this device involves combining the haptic feedback from the motor with visual feedback. In order to provide visual feedback, we plan on mounting a laser to sit on the top of the foot. The laser will also be controlled through the app, thus both the hardware and software will need to be updated to accommodate the addition.

